

1/13

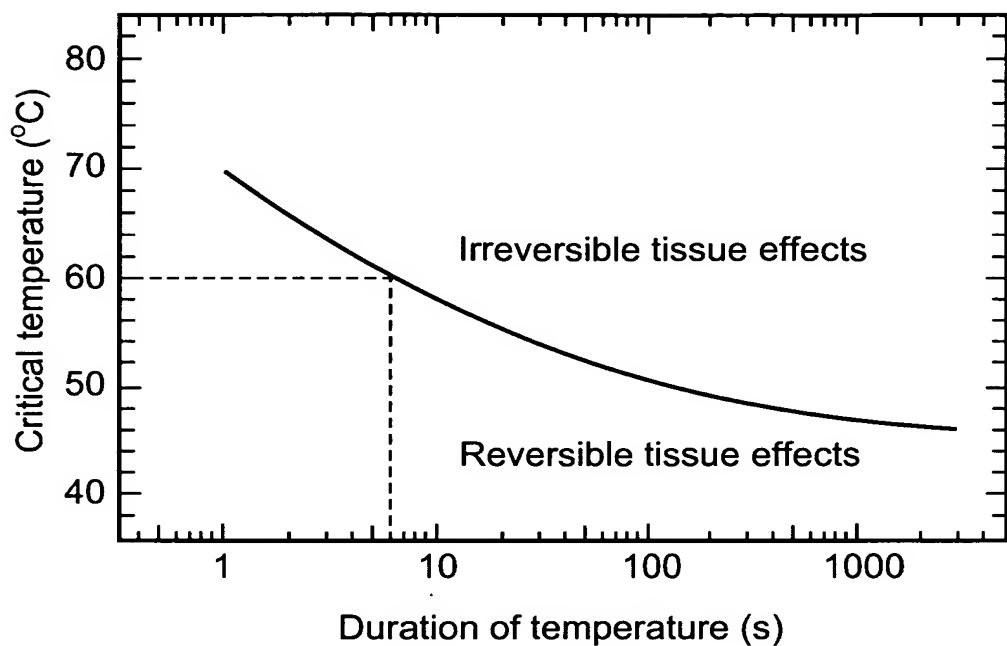


Fig. 1

2/13





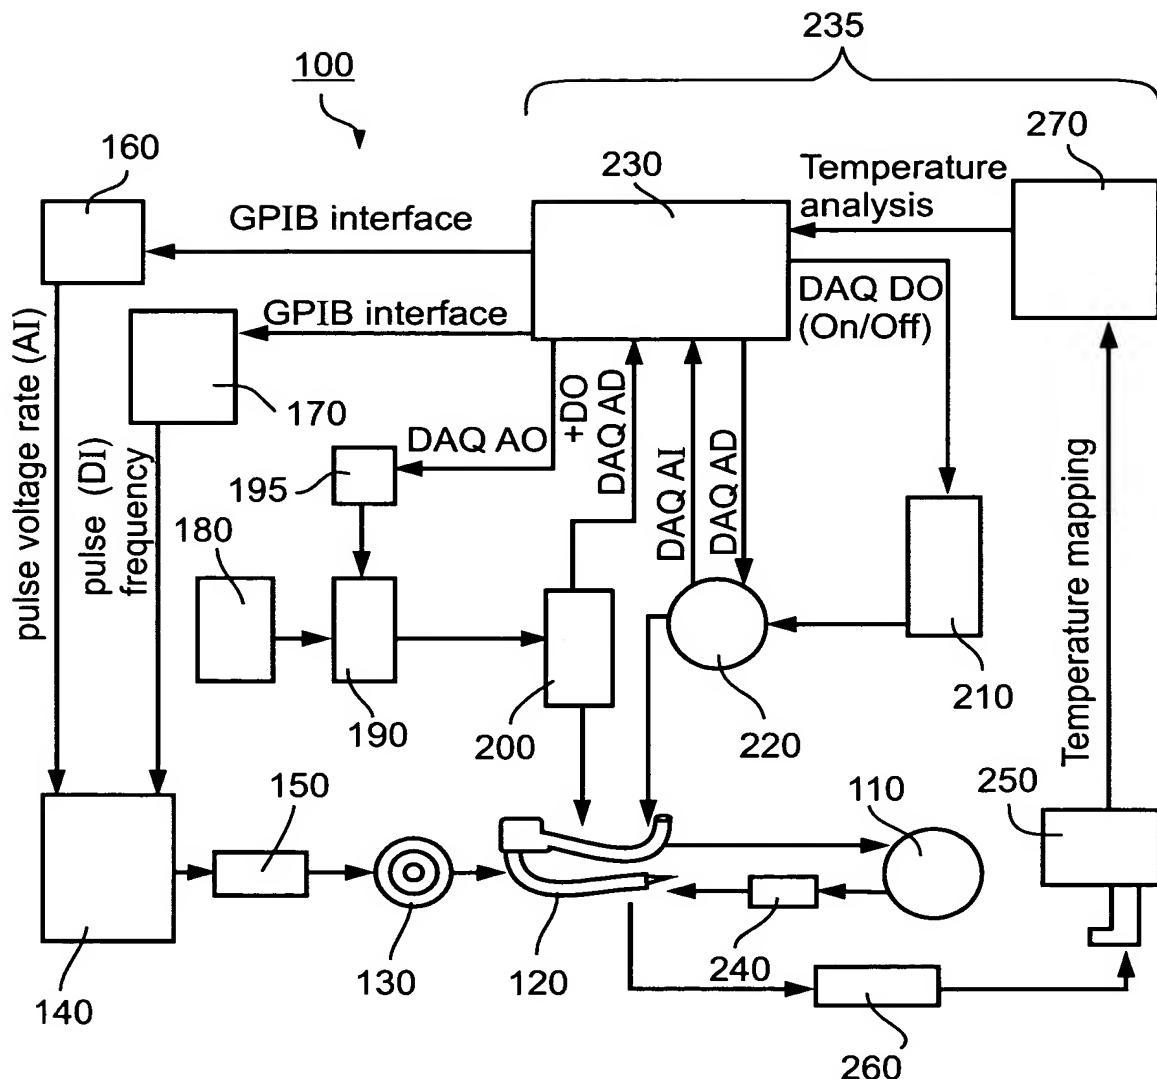


Fig. 2

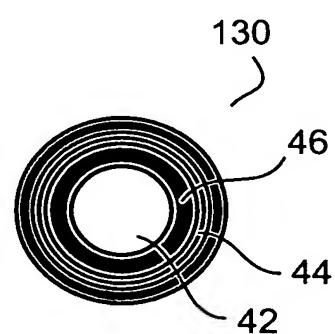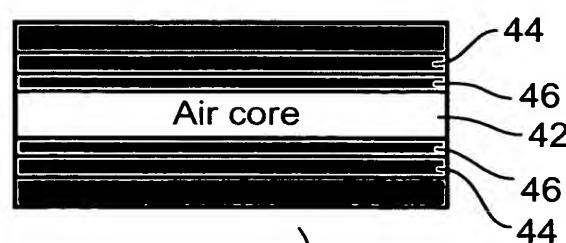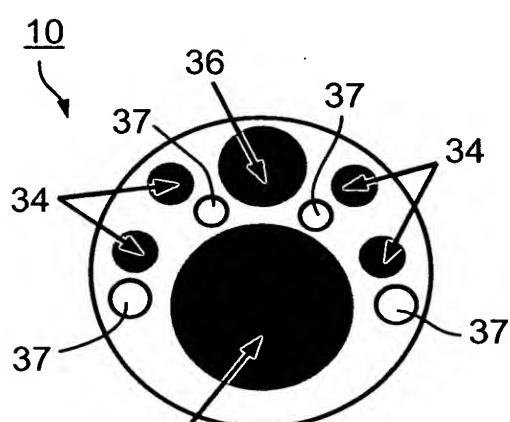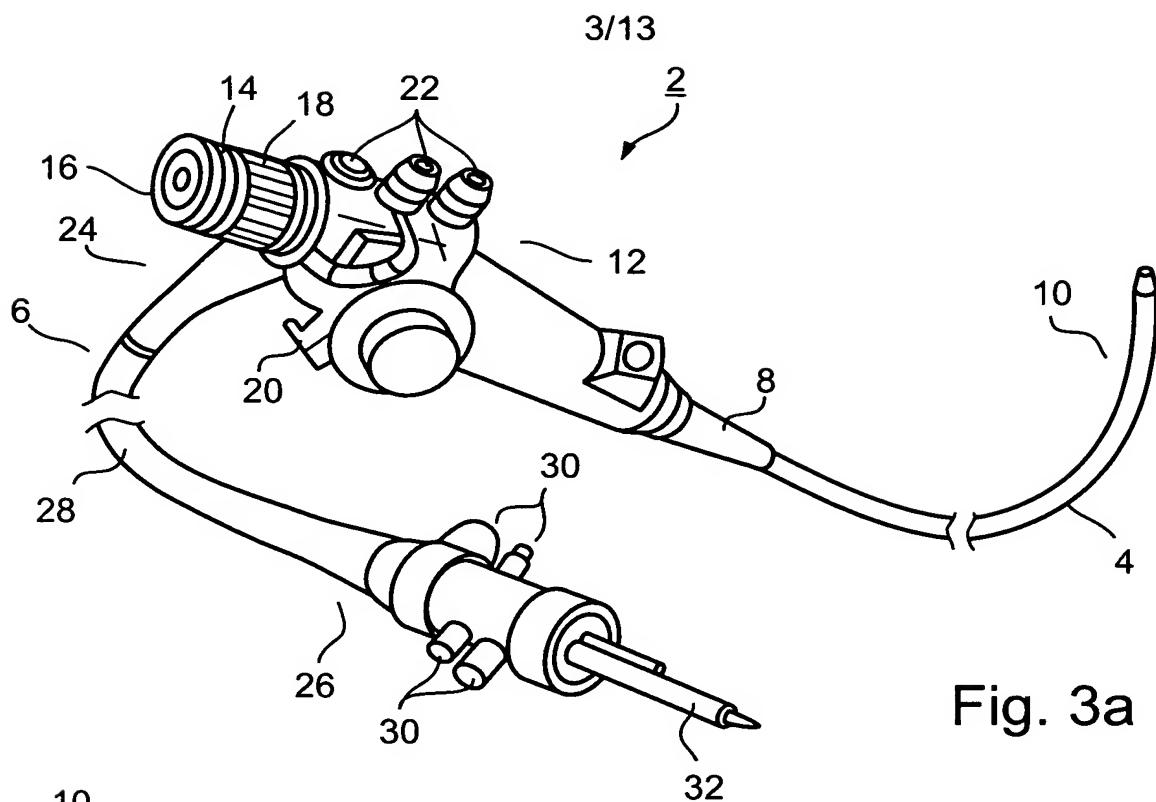

4/13

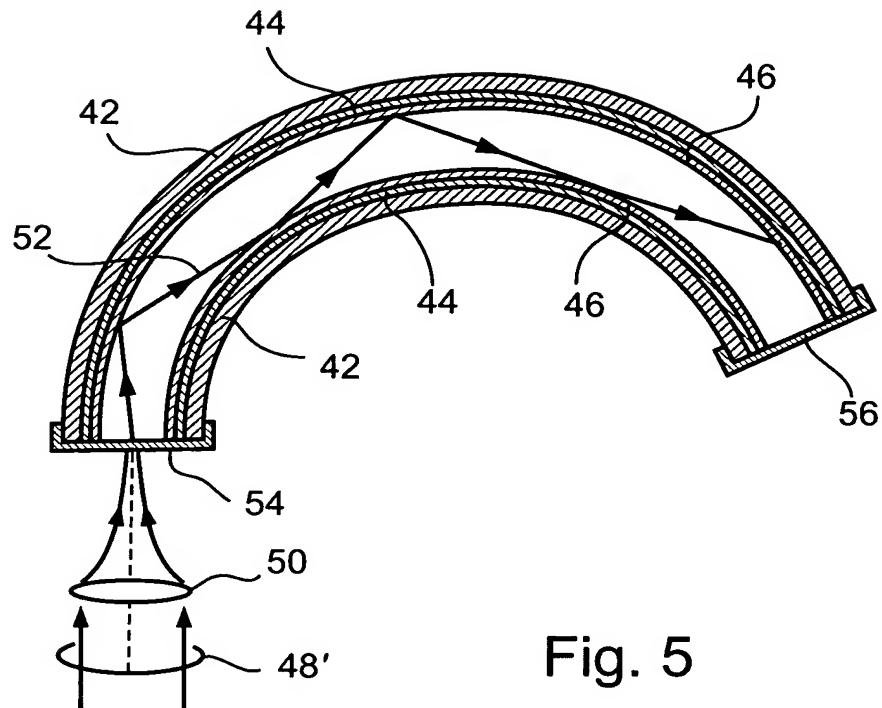


Fig. 5

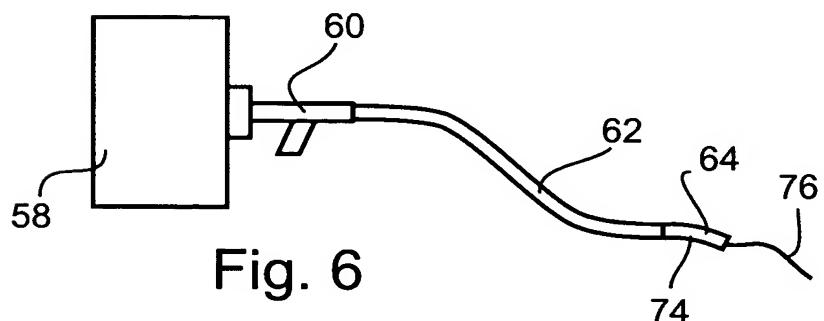


Fig. 6

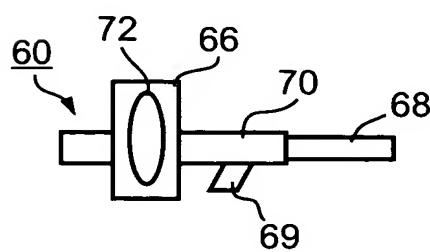


Fig. 7

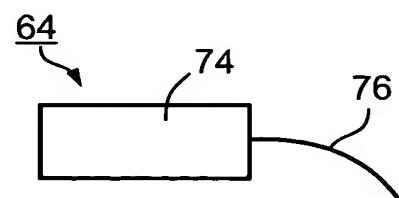


Fig. 8

5/13

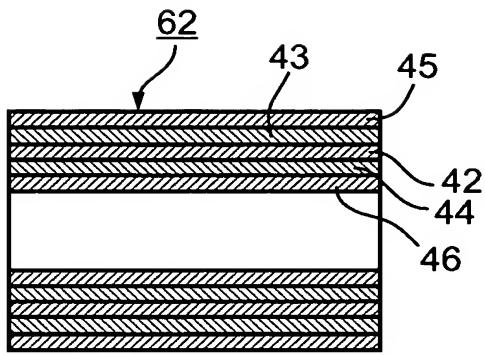


Fig. 9

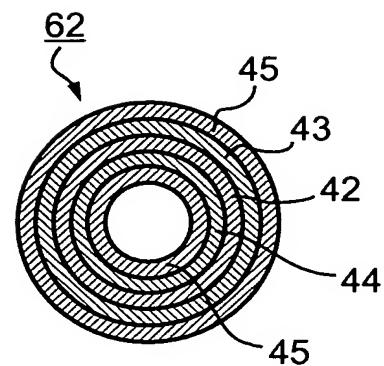


Fig. 10

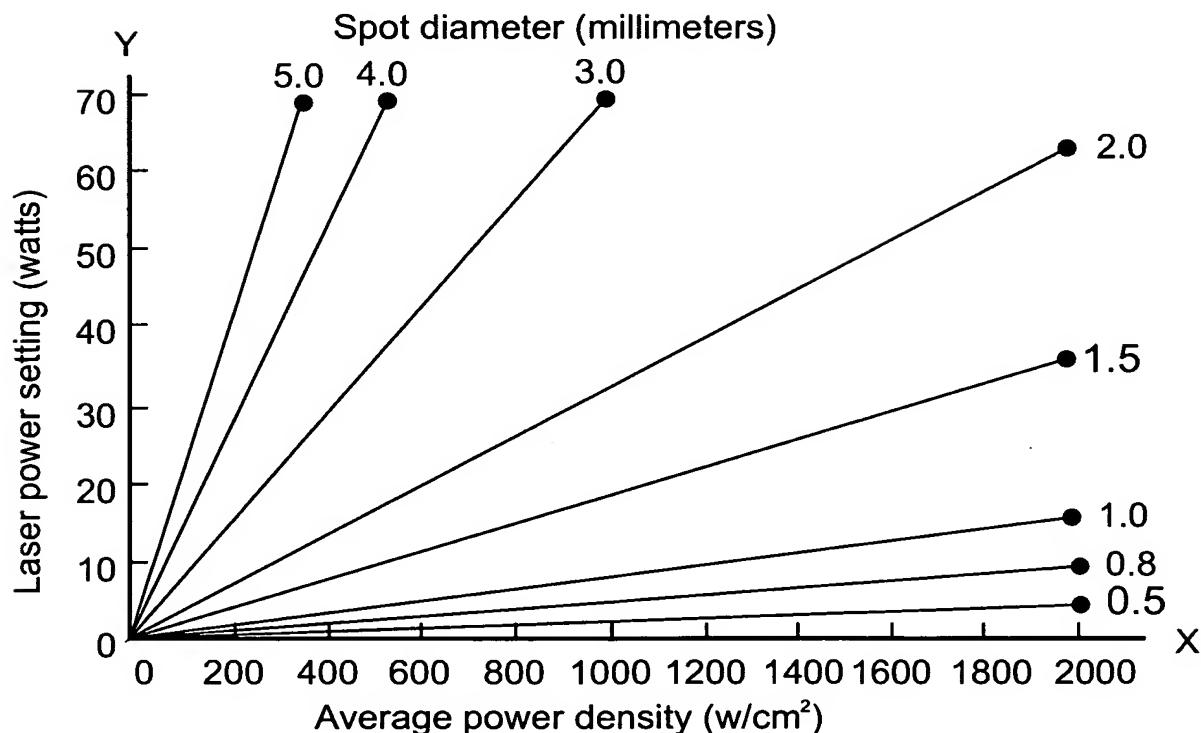


Fig. 11

6/13

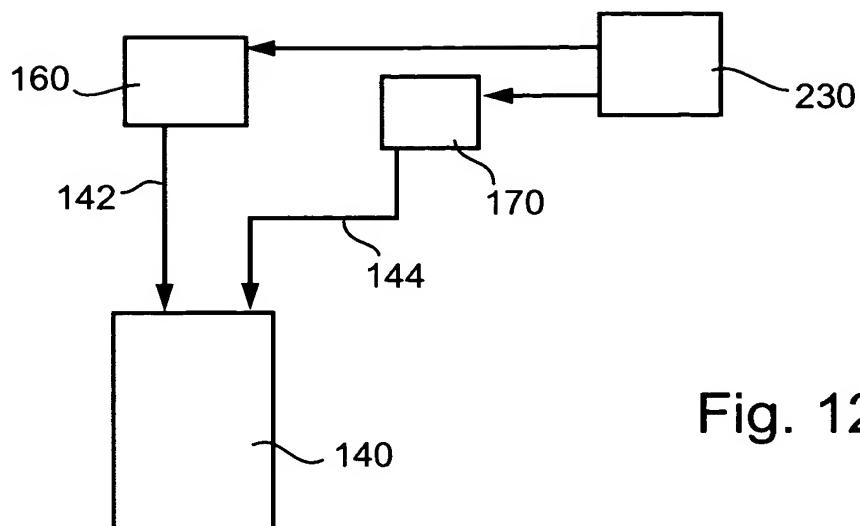


Fig. 12

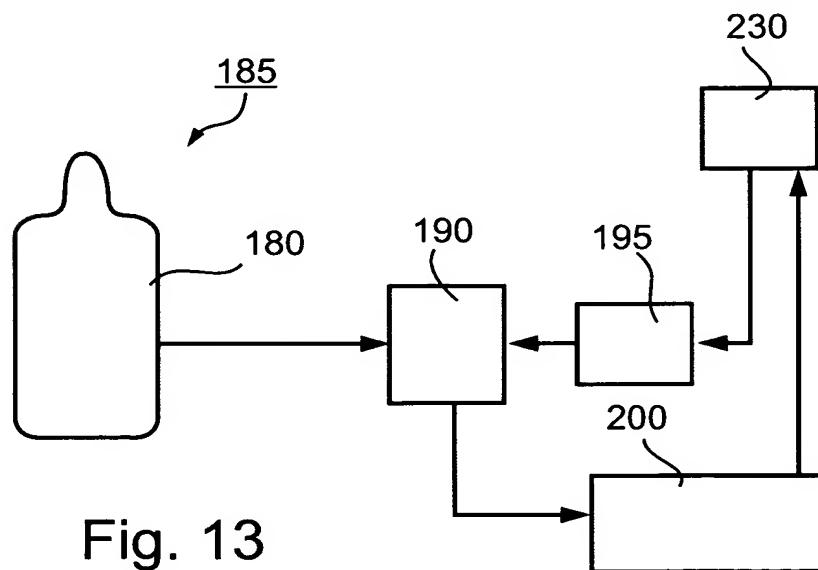


Fig. 13

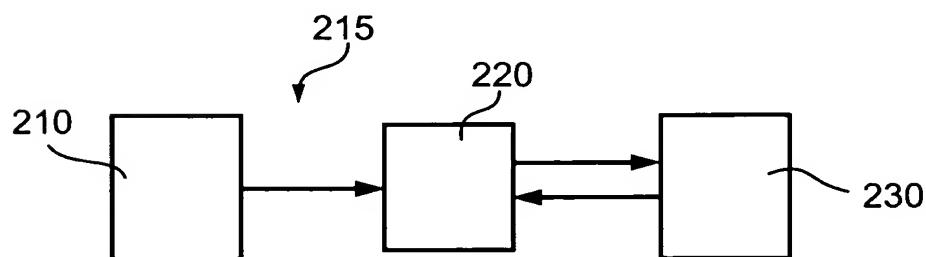


Fig. 14

7/13

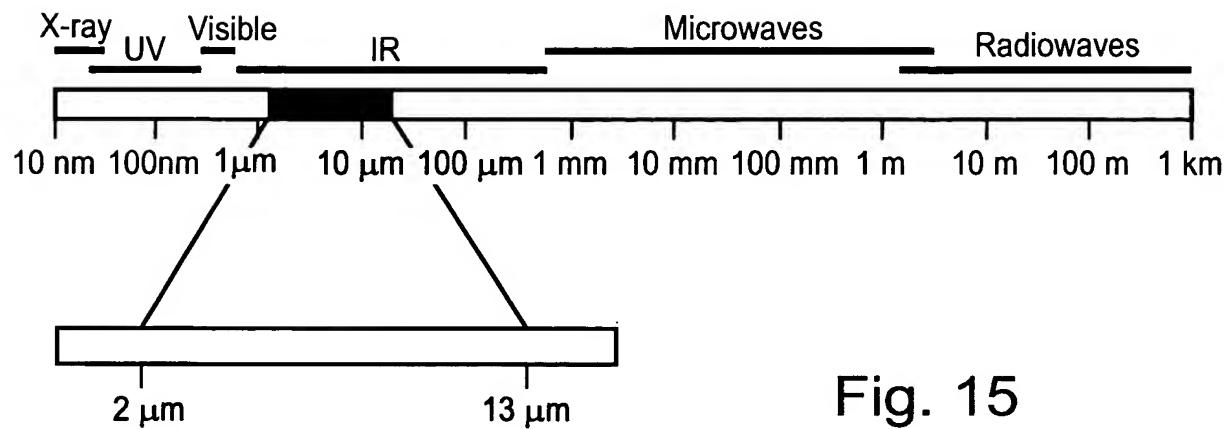


Fig. 15

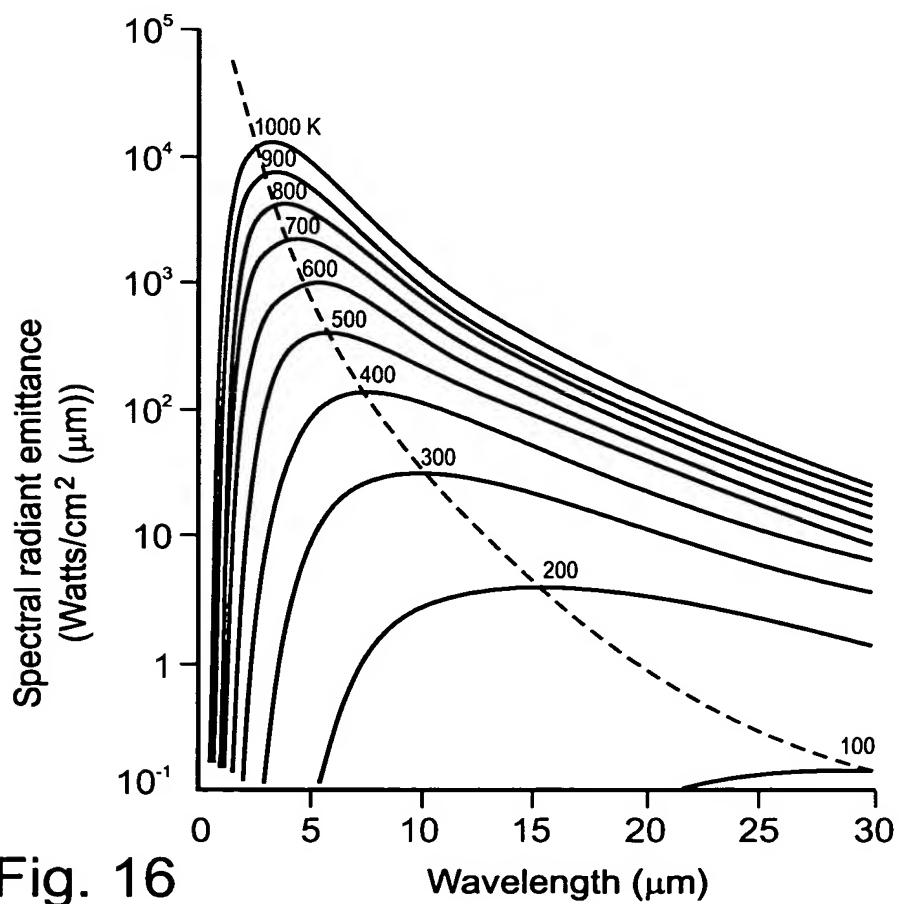


Fig. 16

8/13

Fig. 17



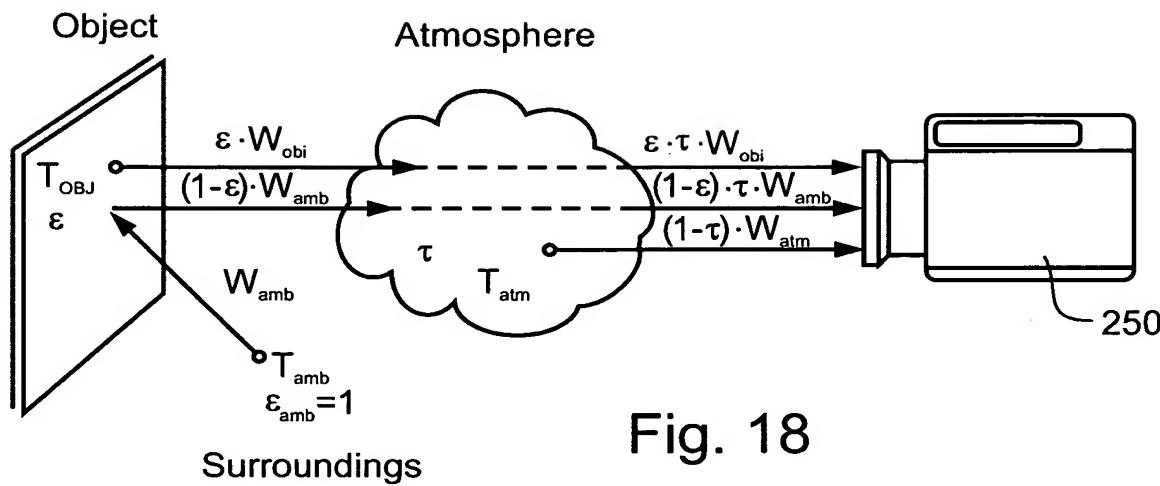


Fig. 18

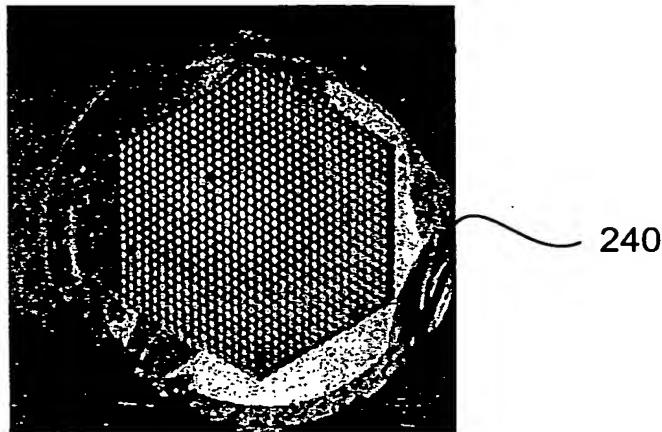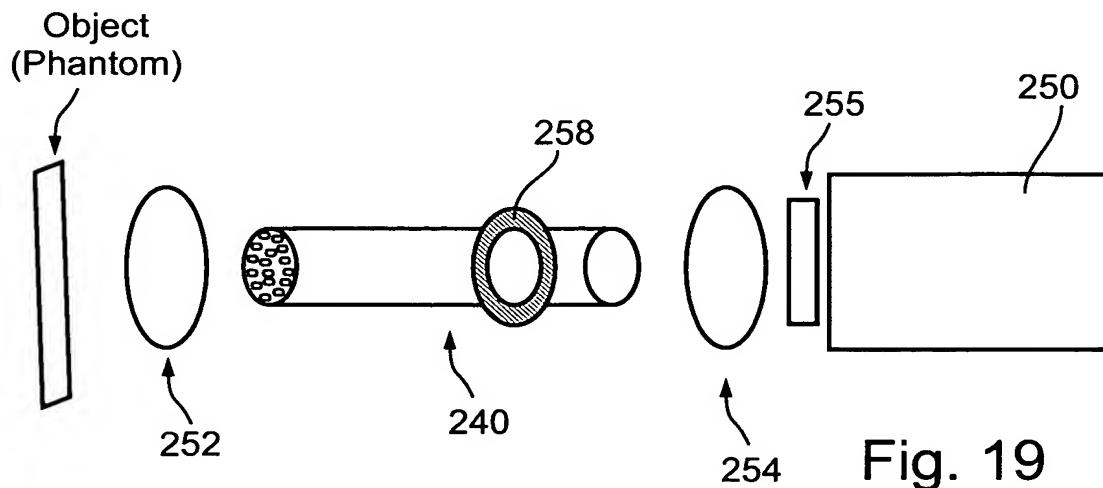

10/542926

Rec'd PCT/PTO 21 JUL 2005

9/13

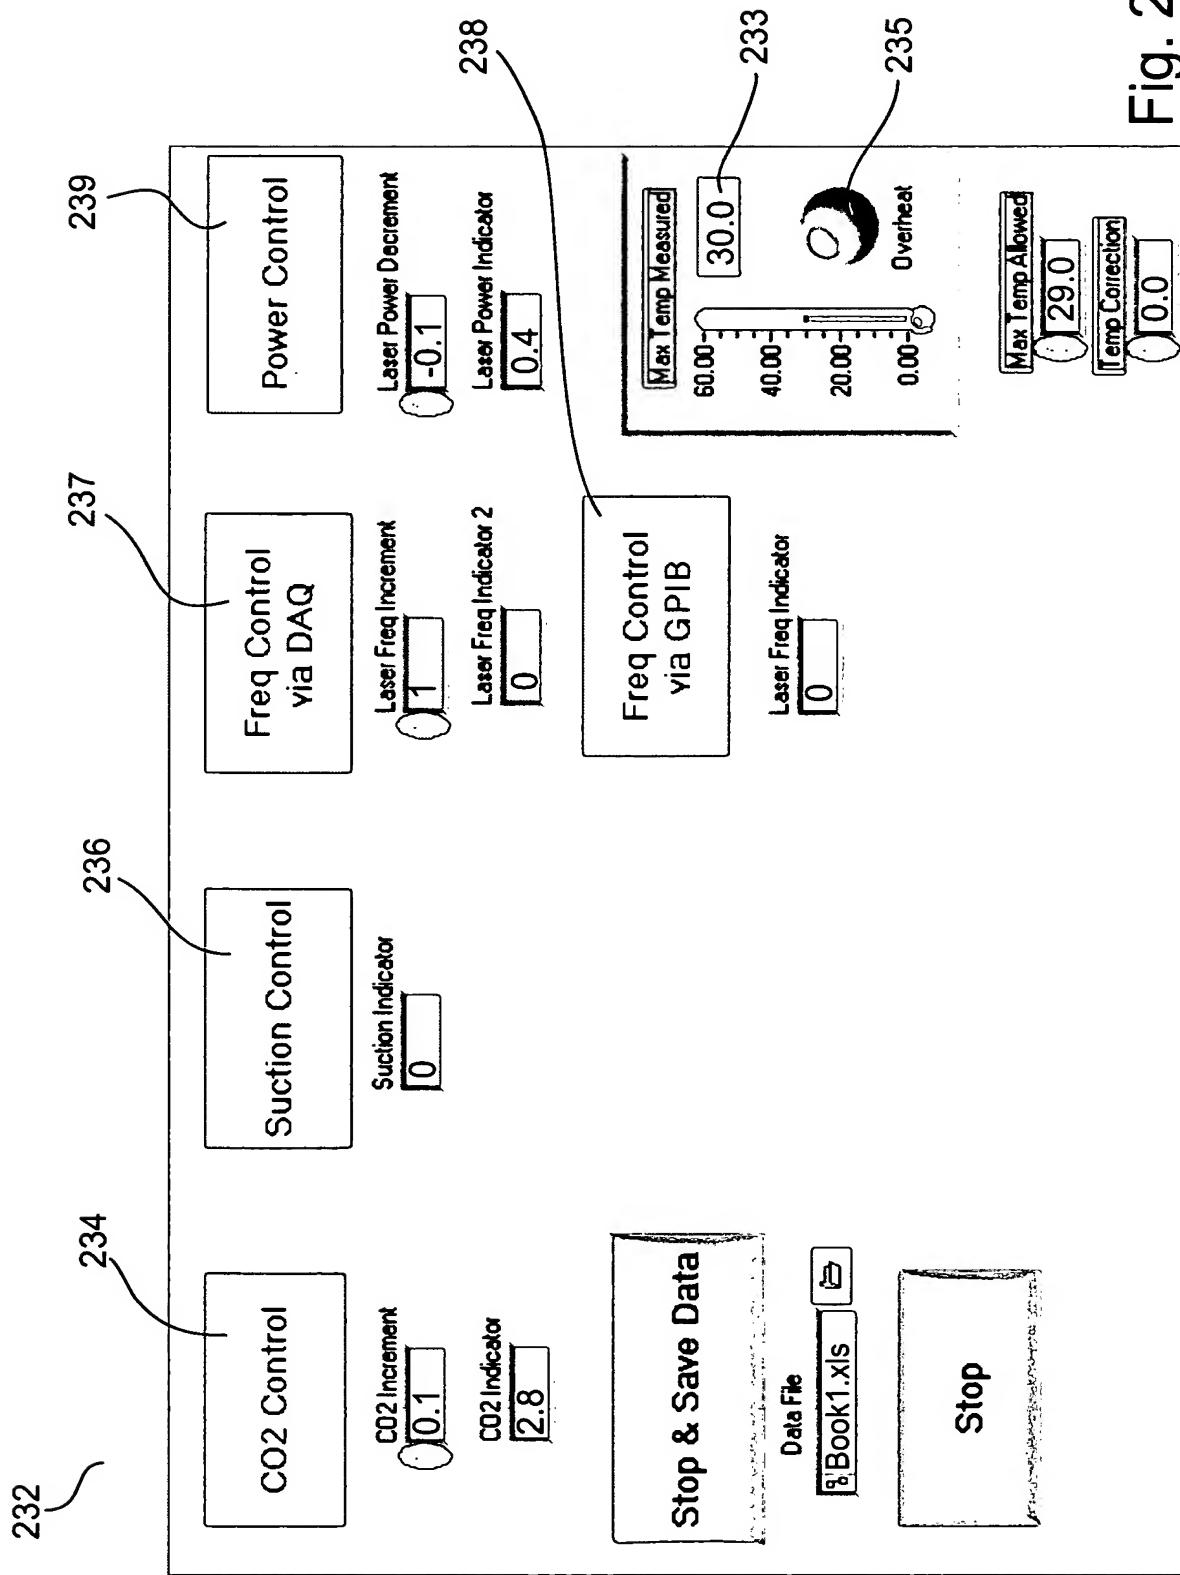


Fig. 20

10/15 42926  
Rec'd PCT/PTO 21 JUL 2005

10/13

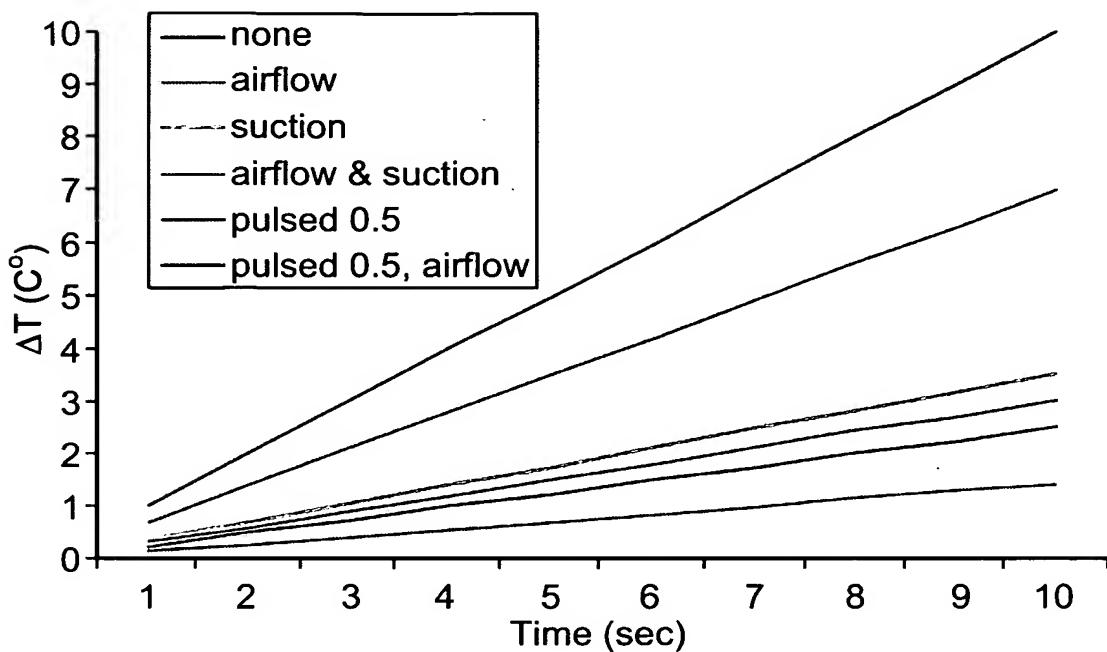


Fig. 21

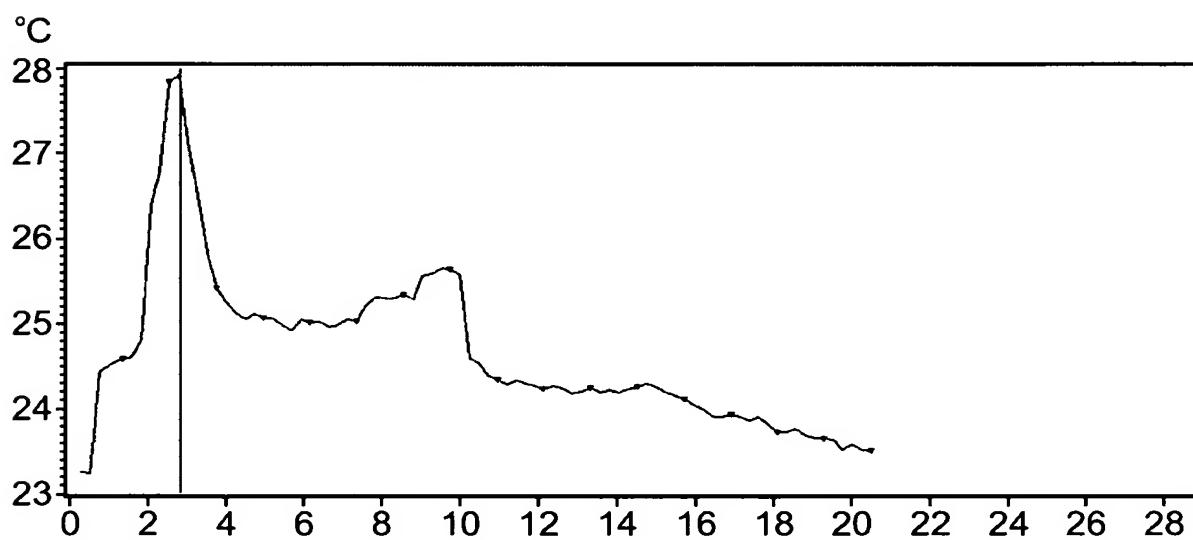


Fig. 22

10/542926

Rec'd PCT/PTO 21 JUL 2005

11/13

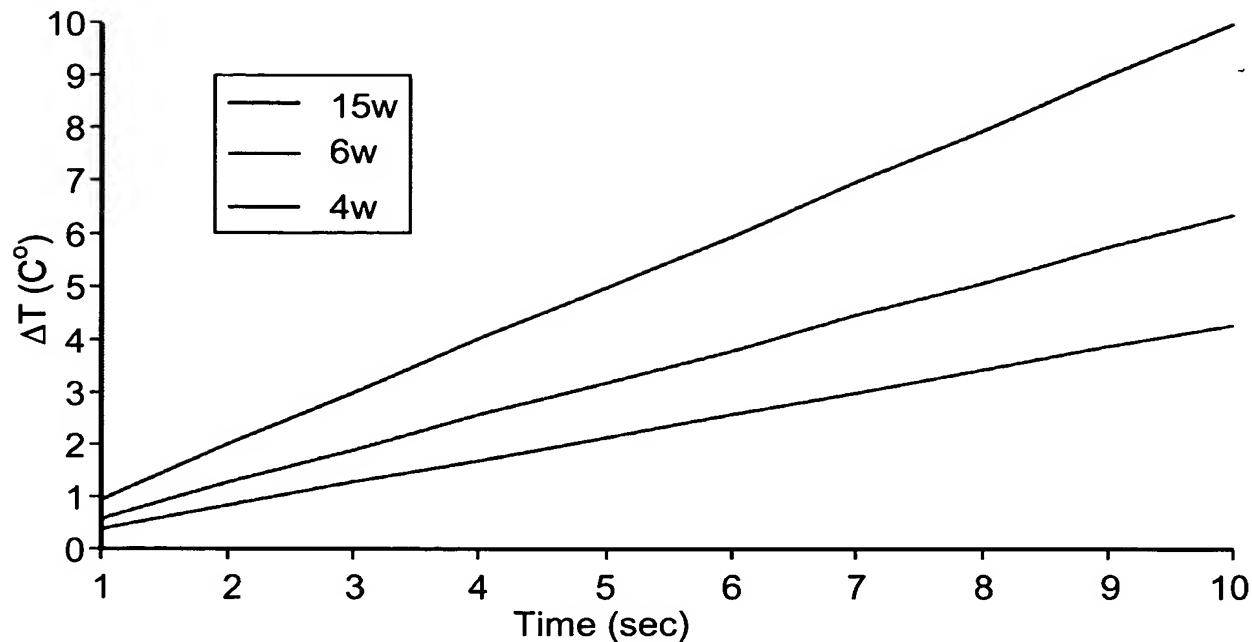


Fig. 23

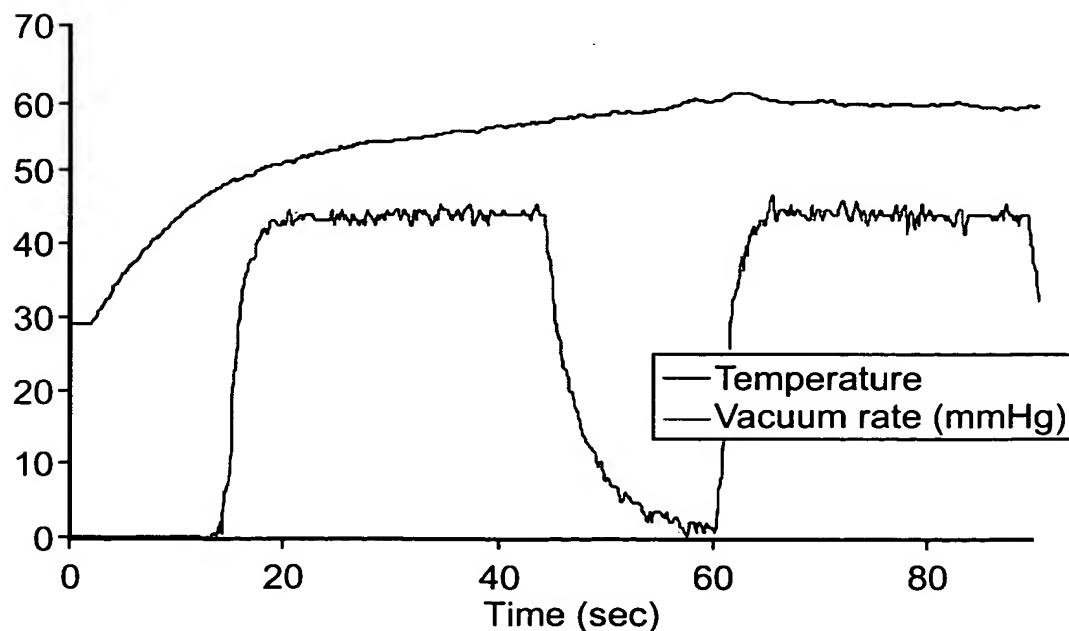


Fig. 24

10/542926  
Rec'd PCT/PTO 21 JUL 2005

12/13

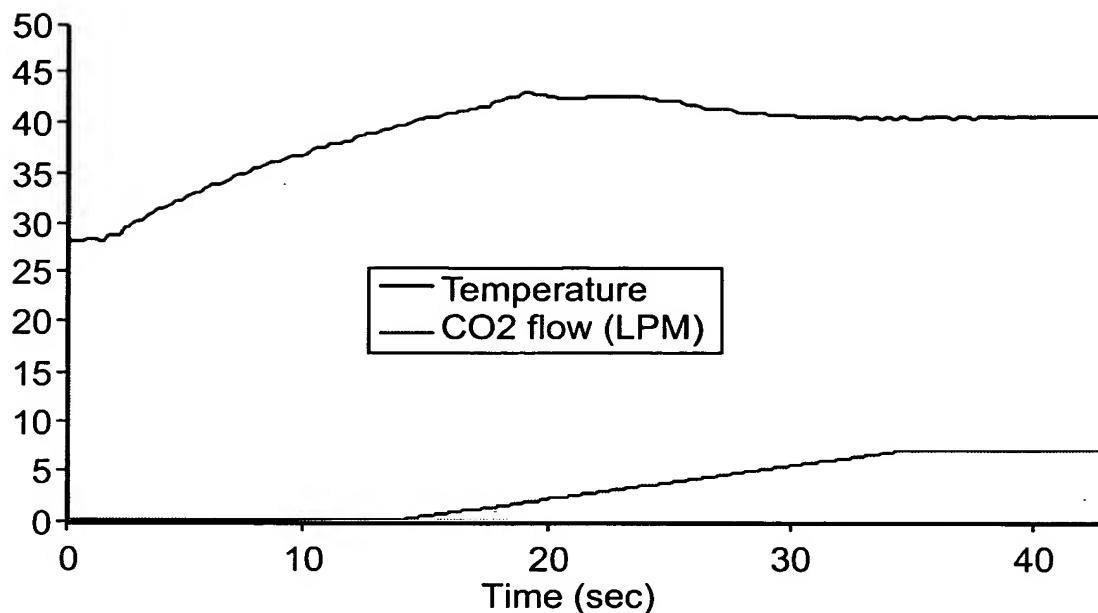


Fig. 25

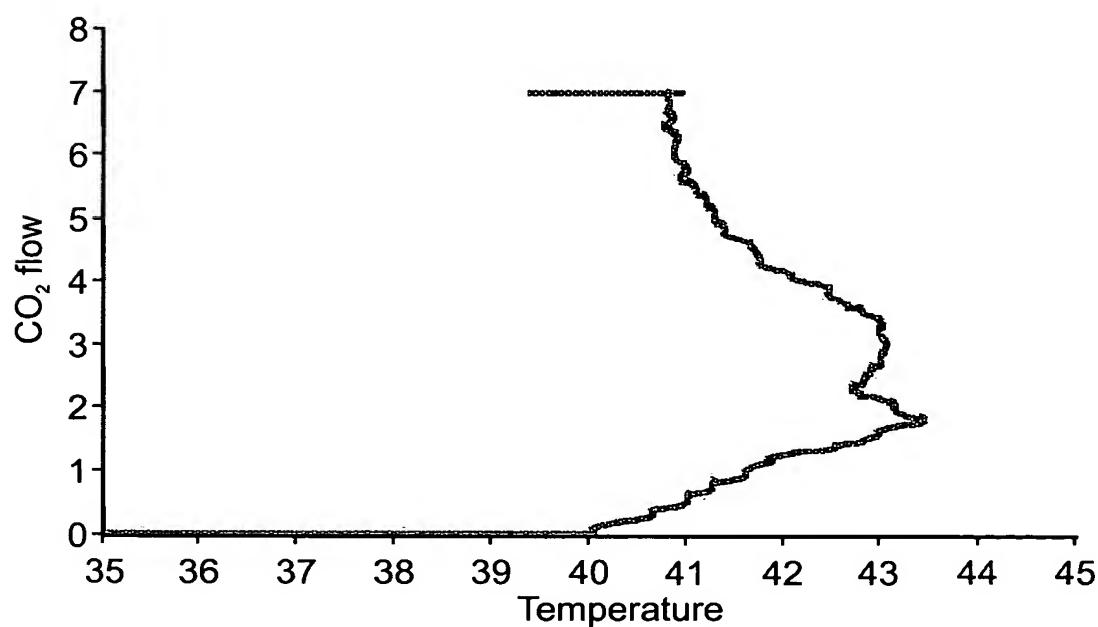


Fig. 26

10/542926

Rec'd PCT/PTO 21 JUL 2005

13/13

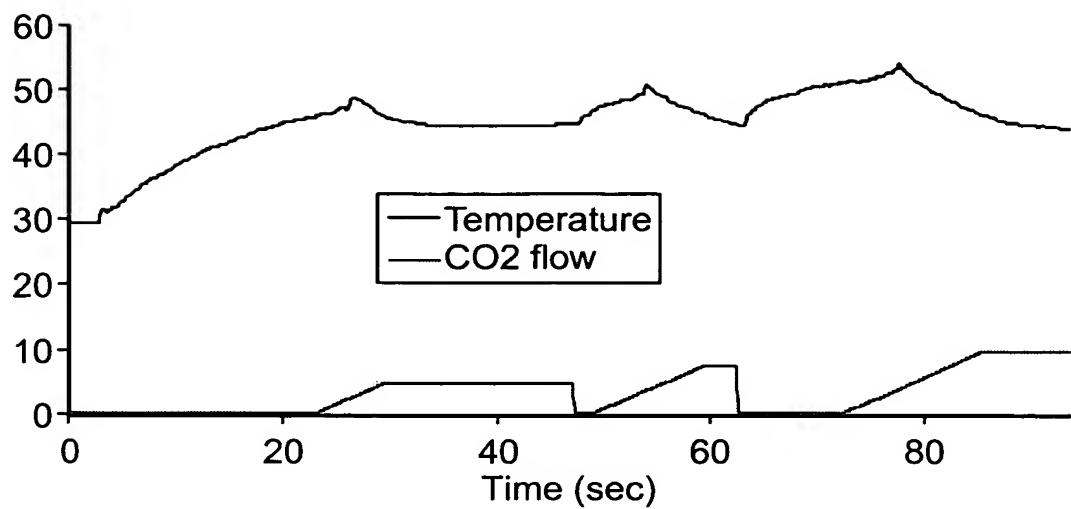


Fig. 27